


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

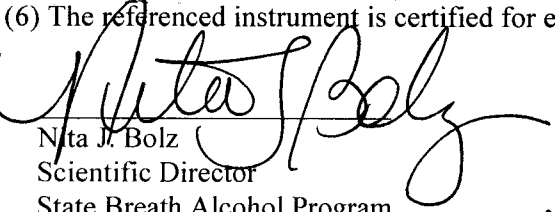
DEC 07 2009

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130187 ✓
Name	Dan Pasquariello	ID#	2620
		Date	12-02-09 ✓
A	Agency	Dillingham PD	Phone # 842-5354
	Instrument Location	Dillingham PD ✓	
B	Alco S/N	78853 ✓	Target Value .083 ✓
			High Pressure 700 psi
	Alco Test Value Average	.080 ✓	.080 ✓
		1 st Alco	2 nd Alco
	Signature	 ✓	08/12/09
(OVER)			

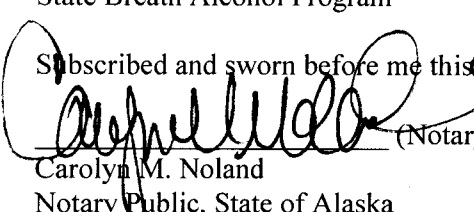
(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 31st day of Dec, 2009.


(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130187 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130187 ✓

DECEMBER 02, 2009 ✓ *COB 12/2/09*

OPERATOR'S NAME:

PASQUARIELLO, DAN

OPERATOR'S NUMBER: 2628

SUBJECT'S LAST NAME:

UOC

SUBJECT'S FIRST NAME/MI :

UOC

O.L. #: 1234567890

DEPT/AGENCY: DL61

CASE/REPORT: 1234567890

TEST TYPE: U

ALCO TARGET VALUE: .003 ✓

ALCO S/N: 78853 ✓

— BREATH ANALYSIS —

.003 ADJUSTED FOR 29.33 in ✓

ALCO TARGET .001 12:06

BLANK TEST .000 12:07

INTERNAL STANDARD VERIFIED 12:07

ALCO TV 29.33 in .000 ✓ 12:08

BLANK TEST .000 12:09

SUBJECT SAMPLE *COB 12/2/09* .000 12:09

BLANK TEST .000 ✓ 12:10

ALCO TV 29.33 in .000 12:10

BLANK TEST .000 12:11

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130187

DECEMBER 02, 2009 ✓

TIME 12:12

— DIAGNOSTIC CHECK —

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 43c

BREATH TUBE: 42c

BAROMETER: 29.33 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z () * +